



Contents lists available at ScienceDirect

Journal of the Mechanical Behavior of Biomedical Materials

journal homepage: www.elsevier.com/locate/jmbbm

Characterisation of human urethral rupture thresholds for urinary catheter inflation related injuries

N.F. Davis^{a,*}, E.M. Cunnane^{b,1}, R.O.'C. Mooney^b, J. Hess^c, M.T. Walsh^b^a Department of Urology and Transplant Surgery, Beaumont Hospital, Dublin, Ireland^b Centre for Applied Biomedical Engineering Research, School of Engineering, Bernal Institute and the Health Research Institute, University of Limerick, Limerick, Ireland^c Department of Urology, University Hospital Essen, University Duisburg-Essen, Germany

ARTICLE INFO

Keywords:

Urethral trauma
Urethral injury
Urinary catheter
Urethral rupture

ABSTRACT

Data on urethral catheter related injuries is sparse. In this study we aimed to characterise urethral diametric strain and urinary catheter inflation pressure thresholds that precede human urethral trauma during urethral catheterisation (UC). Human urethras were obtained from patients undergoing male to female gender re-assignment surgery [(n = 9; age 40 ± 13.13 (range: 18–58)) years]. 12Fr urinary catheters were secured in the bulbar urethra and the catheter's anchoring balloon was inflated with a syringe pump apparatus. Urethral diametric strain and balloon pressure were characterised with video extensometry and a pressure transducer respectively. Immunohistochemistry, Masson's trichrome and Verhoeff-Van Gieson stains evaluated urethral trauma microscopically. Morphological characterisation of the urethral lumen was performed by examining non-traumatised histological sections of urethra and recording luminal area, perimeter and major/minor axis length. Tearing (n = 3) and rupture (n = 3) of the urethra were observed following catheter balloon inflation. The threshold for human urethral rupture occurred at an external urethral diametric strain ≥ 27% and balloon inflation pressure ≥ 120kPa. Significant relationships were identified between urethral wall thickness and the level of trauma induced during catheter balloon inflation (p = 0.001) and between the pressure required to inflate the catheter balloon and the length of the major axis of the urethral lumen (p = 0.004). Ruptured urethras demonstrated complete transection of collagen, elastin and muscle fibres. In conclusion, urethral rupture occurs at an external urethral diametric strain ≥ 27% or with balloon inflation pressures ≥ 120 kPa. Incorporation of these parameters may be useful for designing a safety mechanism for preventing catheter inflation related urethral injuries.

1. Introduction

Approximately 25% of hospitalised patients undergo urethral catheterisation (UC) during their inpatient stay (Davis et al., 2017a). Of these, 0.3–0.7% will sustain iatrogenic urethral trauma secondary to inadvertent inflation of the catheter's anchoring balloon in the urethra (Sullivan et al., 2014; Thomas et al., 2009). Short-term complications associated with traumatic UC are penile/perineal pain, urosepsis, acute urinary retention, urethral bleeding or urinary tract infection (Davis et al., 2017a). Long-term complications include urethral stricture disease with subsequent reconstructive procedures (Thomas et al., 2009; Kashefi et al., 2008). Despite these preventable iatrogenic morbidities, few studies examine mechanisms to prevent UC related injuries (Simhan, 2015). Of those that examine such mechanisms, none are

based on data obtained from testing of human urethras (Davis et al., 2015). This study seeks to characterise the relevant mechanics of human urethral tissue in order to further develop mechanisms to prevent urinary catheter related injuries. To achieve this the urethral diametric stretch and catheter balloon inflation pressure thresholds that precede human urethral injury are characterised during intentional inflation of a urinary catheter anchoring balloon in the bulbar urethra of explanted human male urethras.

2. Methods

2.1. Patient characteristics

Following hospital ethical research committee approval, human

Abbreviations: OD, Outside diameter; ID, Inside diameter; UC, Urethral catheterisation

* Corresponding author.

E-mail address: nialldavis@rcsi.ie (N.F. Davis).

¹ Denotes joint first authorship.

<https://doi.org/10.1016/j.jmbbm.2018.04.015>

Received 26 February 2018; Received in revised form 17 April 2018; Accepted 17 April 2018

Available online 19 April 2018

1751-6161/ © 2018 Elsevier Ltd. All rights reserved.

urethras were obtained from 9 consenting patients undergoing male to female gender reassignment surgery at the University Hospital Essen, Essen, Germany. The mean age was 40 ± 13.13 years (range: 18–58 years). Samples were maintained at *in vivo* length by tethering the urethra to a urinary catheter during surgical excision. All samples included the bulbar urethra at the proximal end, the penile urethra and the glans of the penis at the distal end. The glans was excised prior to testing to facilitate mounting of the samples in a custom fabricated catheter inflation apparatus.

2.2. Preparation of human urethras

Human urethras were stored at -20°C within 2 h of excision. This method of storage was employed as it has been previously demonstrated to have no significant effects on biological soft tissue mechanical properties once the tissue is unfrozen (Ebenstein et al., 2009; O'Leary et al., 2014). Prior to testing, samples were defrosted overnight at 4°C and subsequently immersed in distilled water at 37°C to equilibrate the tissue back to physiological temperature on the day of testing. Prior to testing, *in vivo* length and external diameter of samples was measured using Vernier callipers. Measurements were confirmed using a non-contact photography method. The mean *in vivo* length of the samples was 147.44 ± 13.97 mm (range: 122.96–167.76 mm). Samples were then marked with acrylic paint at points 5 cm from each end. This distance was then measured to allow for restoration of samples to *in vivo* length and to ensure proper alignment of the samples in the catheter inflation apparatus.

2.3. Catheter-inflation testing

Samples were mounted in the apparatus demonstrated in Fig. 1. Physiological humidity and temperature were achieved during testing by submersing the samples in a distilled water bath maintained at 37°C . Each end of the sample was mounted on stainless steel tubular mounts (OD = 6.5 mm, ID = 5 mm) lined with 60 grit sandpaper and secured with wire hose clips of internal diameter ranging from 9 to 13 mm. Samples were then aligned and restored to *in vivo* length. A 12Fr Coloplast® silicone urinary catheter was inserted into the sample *via* the proximal hollow tubular mount and the tip was secured in a recess in the distal mount. This method ensured that the anchoring balloon of the catheter was in the bulbar urethra prior to inflation. The anchoring balloon was then inflated with 10 ml of saline *via* a syringe (BD, USA) and a syringe pump (Pump Systems Inc., USA, Model: NE-1000) at an

inflation rate of 30 ml/min (Davis et al., 2015). No more than 10 ml of saline was injected into each catheter anchoring balloon as to do so would not be clinically representative. The resulting pressure was monitored using a calibrated 1 bar pressure transducer (Sensortechnik, USA). The corresponding change in sample outer diameter was monitored using a video extensometer (Messphysik, Austria).

2.4. Histology and immunohistochemistry

Masson's trichrome and Verhoeff-Van Gieson stains were employed to histologically evaluate trauma to epithelium, collagen and elastin within the urethral extracellular matrix (ECM) following testing. Small ring segments (approx. 5 mm) were cut from the traumatised region and adjacent non-traumatised region of samples and fixed traction-free in 10% formalin, embedded in paraffin, and then sliced into 10 μm thick segments. Immunohistochemical staining of muscle actin was also used to identify the smooth and striated muscle content of the samples. Images of the stained samples were obtained using a Nikon microscope (Eclipse, 90i) at $4\times$ and $20\times$ for gross and detailed imaging respectively. The composition of each sample was assessed from the histological images using a previously outlined protocol which employs ImageJ to convert collagen composition to the mean Gray value of the blue colour intensity of the Mason's Trichrome stains with respect to tissue area (Bauman et al., 2014). This protocol uses hue (121–179), saturation (20–255) and brightness (10–255) to isolate collagen from stained images and is also adapted for elastin and muscle content. Both elastin and muscle content are identified using the YUV colour space (elastin: $Y = 0-120$, muscle: $Y = 0-145$, both: U and $V = 0-255$). Morphological characterisation of the sample lumen was performed by examining the adjacent non-traumatised histological sections using ImageJ and recording lumen area, perimeter and major/minor axis length. Major and minor axis lengths consider the profile of the sample lumen to be an ellipse and refer to the maximum and minimum diameter of this ellipse respectively.

2.5. Statistical analysis

Statistical analysis was performed using Minitab 17 (Minitab Inc. State College, PA, USA). Correlations between the variables were assessed using 2-tailed parametric bivariate analysis and regression analysis was performed to examine the relationship between these variables. Statistically significant differences were identified between groups of continuous variables using 2-tailed *t*-tests. A *p* value < 0.05

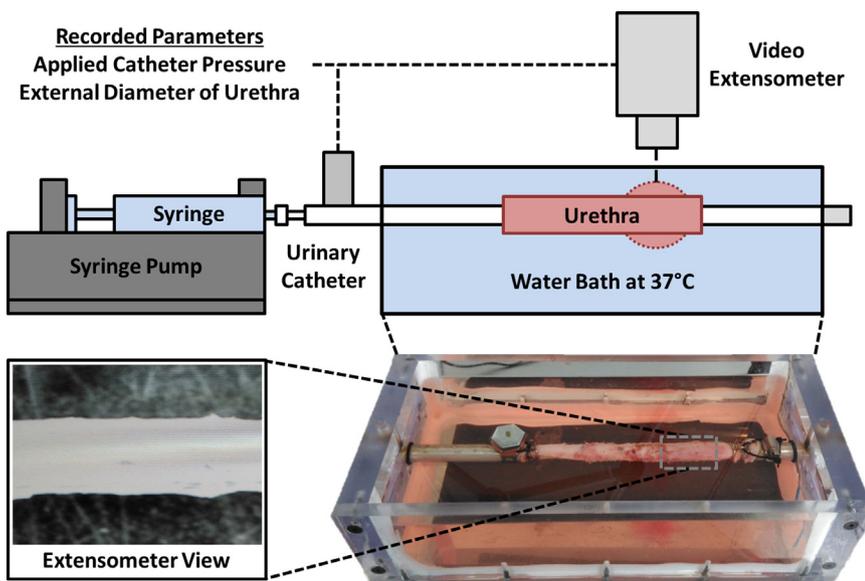


Fig. 1. Schematic of the experimental apparatus used to perform inflation testing of urinary catheters in human urethral samples. Male explanted urethras were mounted on stainless steel tubular mounts and secured. Samples were then aligned and restored to *in vivo* length. A 12Fr silicone urinary catheter was inserted and secured in a recess in the distal mount to ensure that the anchoring balloon of the catheter was in the bulbar urethra prior to balloon inflation. The anchoring balloon was then inflated with 10 ml of saline *via* a syringe and a syringe pump.

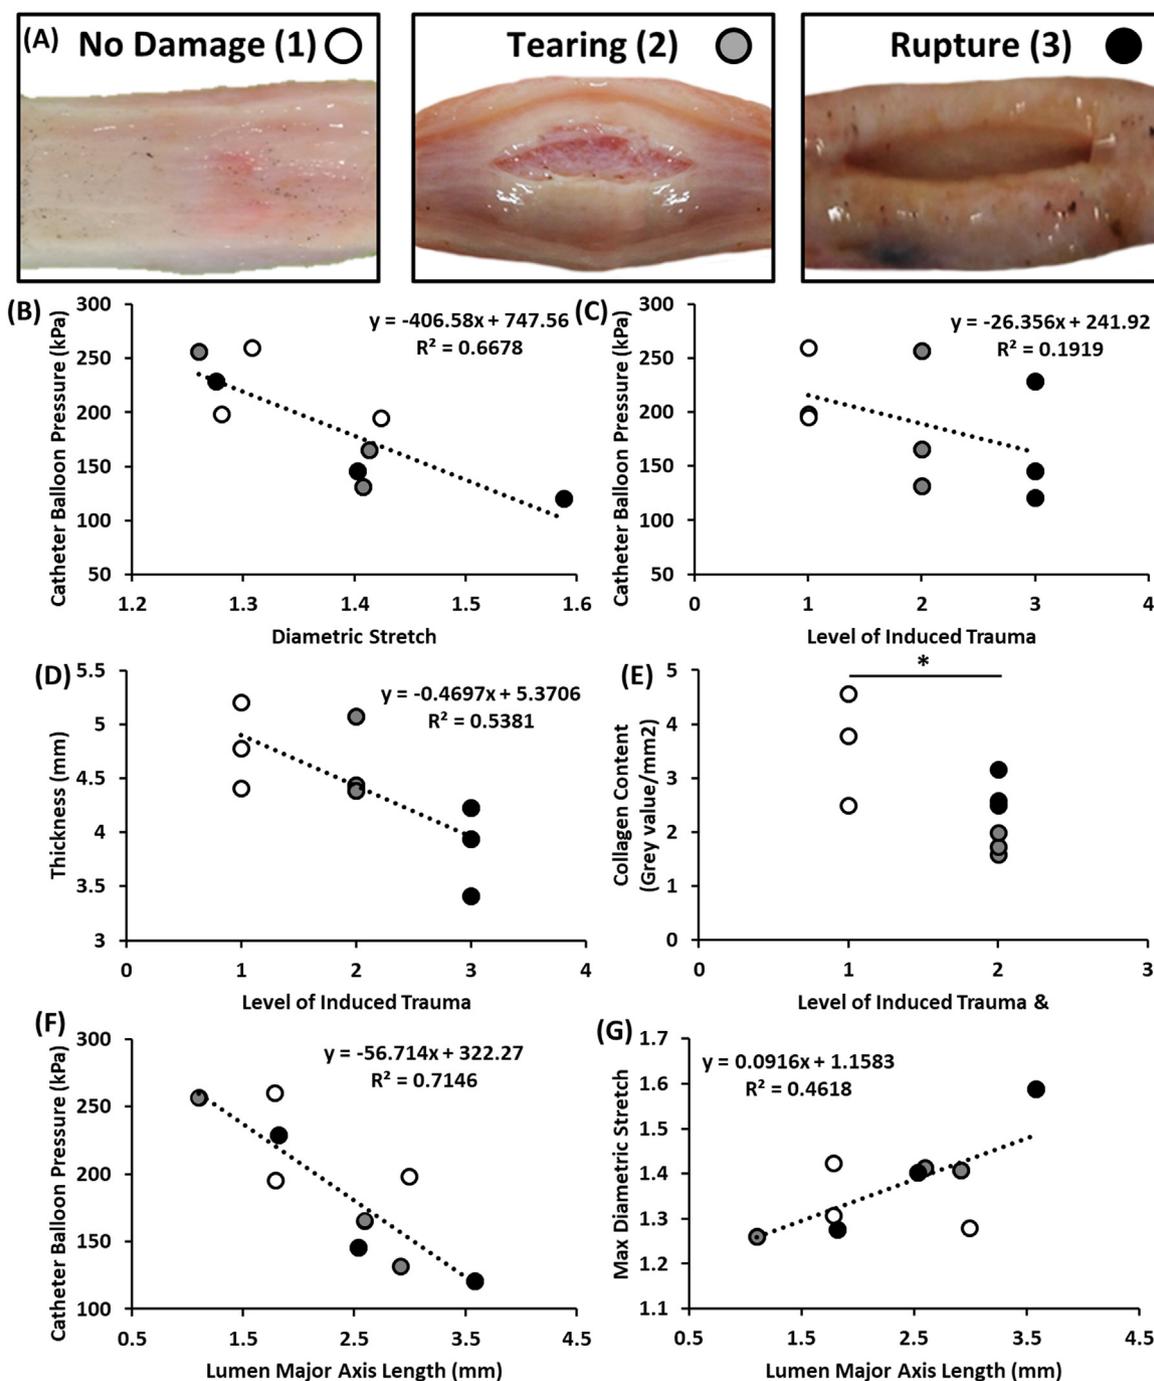


Fig. 2. A) Representative images of urethra samples that experienced no damage (n = 3), tearing (n = 3) and rupture (n = 3) following inflation of a urinary catheter anchoring balloon in the bulbar male urethra. B) Relationship between the maximum external diametric stretch of the sample and the inflation pressure required to inflate the catheter anchoring balloon. C) Relationship between urethral trauma and catheter balloon pressure. 1 corresponds to no damage (open circles), 2 corresponds to tearing (gray circles) and 3 corresponds to rupture (black circles). D) Relationship between urethral trauma and thickness of the urethral wall. E) Significantly higher collagen content identified in samples that experienced no damage compared to those that underwent tearing or rupture. F) Relationship between the maximum external diametric stretch of the sample and the inflation pressure required to inflate the catheter anchoring balloon. G) Relationship between the pressure required to inflate the catheter anchoring balloon and the length of the major axis of the sample lumen. H) Relationship between the maximum external diametric stretch of the sample and the length of the major axis of the sample lumen.

was considered statistically significant.

3. Results

3.1. Catheter-inflation testing

Two distinct forms of urethral injury were observed following

catheter balloon inflation: rupture (n = 3) and tearing (n = 3) as illustrated in Fig. 2. Rupture is defined as complete separation of urethral tissue and tearing is defined as partial separation of urethral tissue. The type of urethral trauma sustained by each sample, the inflation pressure/diametric stretch at which it occurred, the sample thickness and the length of the lumen major axis are demonstrated in Table 1. Urethral external diametric stretch is calculated as the urethra outer

Table 1

Urethral trauma sustained, the inflation pressure/diametric stretch at which trauma occurred, the sample thickness, the length of the lumen major axis and the collagen content of each sample.

Sample	Trauma type	Inflation pressure (kPa)	External diametric stretch	Wall thickness (mm)	Lumen major axis length (mm)	Collagen content (Gray value/mm ²)
1	None	198.36	1.28	5.21	2.99	2.49
2	None	195.23	1.42	4.78	1.79	3.78
3	None	260.02	1.31	4.41	1.79	4.57
4	Tearing	165.54	1.41	5.07	2.59	1.73
5	Tearing	131.62	1.41	4.44	2.92	1.59
6	Tearing	256.61	1.26	4.39	1.1	1.99
7	Rupture	120.7	1.59	3.41	3.58	2.59
8	Rupture	228.98	1.28	4.23	1.82	2.5
9	Rupture	145.79	1.4	3.94	2.53	3.16

The threshold for human urethral injury occurred at an internal urethral diametric stretch ≥ 1.26 and balloon inflation pressure ≥ 120 kPa. Urethral external diametric stretch was calculated by dividing the urethra outer diameter, at the location of the catheter balloon and at the point of complete balloon inflation, by the original urethra outer diameter, at the same location, prior to balloon inflation.

diameter at the location of the catheter balloon and at the point of complete balloon inflation, divided by the original urethra outer diameter, at the same location, prior to balloon inflation.

Fig. 2 demonstrates the significant relationships identified between the balloon inflation variables and the sample characteristics through parametric bivariate analysis. Fig. 2A displays representative images of samples that underwent no damage ($n = 3$), tearing ($n = 3$) and rupture ($n = 3$) following catheter balloon inflation. Fig. 2B demonstrates the negative relationship between maximum external diametric stretch and the maximum inflation pressure required to inflate the catheter anchoring balloon ($p = 0.007$). This figure also reveals that the threshold values for maximum external urethral diametric stretch and catheter balloon inflation pressure that precede urethral injury (tearing or rupture) for this cohort of samples are 1.26 and 120 kPa respectively. Fig. 2C demonstrates that a significant relationship was not identified between anchoring balloon inflation pressure and the level of urethral trauma. Fig. 2D demonstrates the negative relationship between the level of urethral trauma and the thickness of the urethral wall ($p = 0.001$). Fig. 2E demonstrates the significantly higher collagen content identified in samples that experienced no damage compared to those that sustained injury ($p = 0.038$). No further significant relationships were identified between the level of urethral trauma and any of the remaining sample parameters. Fig. 2F demonstrates the negative relationship between the inflation pressure required to inflate the catheter anchoring balloon and the major axis length of the sample lumen ($p = 0.004$). Fig. 2G demonstrates the positive relationship between maximum diametric stretch and the major axis length of the sample lumen ($p = 0.045$). All additional sample parameters characterised in this study are listed in [Supplementary table 1](#).

3.2. Histological examination

Histological examination was performed to examine the effect of anchoring balloon inflation on the microstructure of the urethral ECM. Sections of the urethra in which the anchoring balloon was inflated are shown in Fig. 3. Fig. 3A demonstrates the gross effects of catheter anchoring balloon inflation on urethral ECM. Fig. 3B evaluates the microscopic structure of urethral tissue samples that sustained no damage following anchoring balloon inflation ($n = 3$). In this group, elastin fibres are dispersed throughout the ECM and are most dense in the middle and inner layers. Long striated muscle fibres are present in the outer layer of the urethra with smooth muscle in the middle layer. Collagen occurs as wavy coiled bundles of fibres in the outer layer of the urethra. Fig. 3C evaluates the microscopic structure of urethral tissue samples that experienced tearing following anchoring balloon inflation ($n = 3$). Elastin, muscle and collagen fibres appear frayed and separated. Fig. 3D evaluates the microscopic structure of urethral tissue samples that ruptured following anchoring balloon inflation ($n = 3$).

Complete disruption and transection of collagen, elastin and muscle fibre is observed in this group. Disruption of the epithelial layer is also evident in the MTC stain (indicated with an arrow).

4. Discussion

This current study investigates the relationship between external urethral diametric stretch, catheter anchoring balloon inflation pressures and urethral trauma during UC in *ex vivo* human urethral models. Results show that urethral injury can occur at external urethral diametric stretch ≥ 1.26 and catheter balloon inflation pressures ≥ 120 kPa. These findings are important as contemporary catheters and catheter syringes have been unchanged for decades and can routinely generate inflation pressures > 700 kPa (Davis et al., 2015, 2017b; Villanueva and Hemstreet, 2008).

This study also characterises and grades urethral trauma macroscopically using visual inspection and microscopically using immunohistochemistry. Two types of urethral injuries are identified, specifically ‘tearing’ and ‘rupture’, due to anchoring balloon inflation within the bulbar urethra. Previously, internal diametric stretch and maximum catheter balloon inflation pressure thresholds have been investigated as indicative parameters for urethral trauma during UC in porcine models. In porcine urethras, internal urethral diametric stretch > 1.6 and/or a maximum anchoring balloon inflation pressure > 150 kPa results in urethral rupture (Davis et al., 2015). In the present study, the minimum pressure value for human urethral rupture is similar at 120 kPa (for the thinnest sample) and the mean balloon inflation pressure in the samples that underwent rupture is 165.16 ± 56.68 kPa (Table 1). These threshold pressure values highlight the dangers inherent with a misplaced anchoring balloon as they are significantly lower than the aforementioned standard UC inflation pressures.

This mechanical urethral data also provides important novel information on urethral distension and pressure profilometry. Considerable variations in urethral lumen major axis length measurements are identified indicating the highly variable anatomy and luminal geometry of the male urethra. As expected, the pressure required to inflate the catheter balloon decreased as urethral lumen major axis length increases. Similarly, maximum external diametric stretch also increases with increasing lumen major axis length. These findings are intuitive as the catheter balloon can undergo increased expansion in a wider urethral lumen before contacting and traumatising urethral tissue. Variations in vessel wall thickness and collagen content account for the spectrum of urethral trauma identified. Thinner urethras were more likely to rupture and thicker urethras were more likely to experience no damage when exposed to the anchoring balloon inflation pressures. This is also intuitive as thicker samples will experience a lower induced stress due to the force of the inflating balloon being

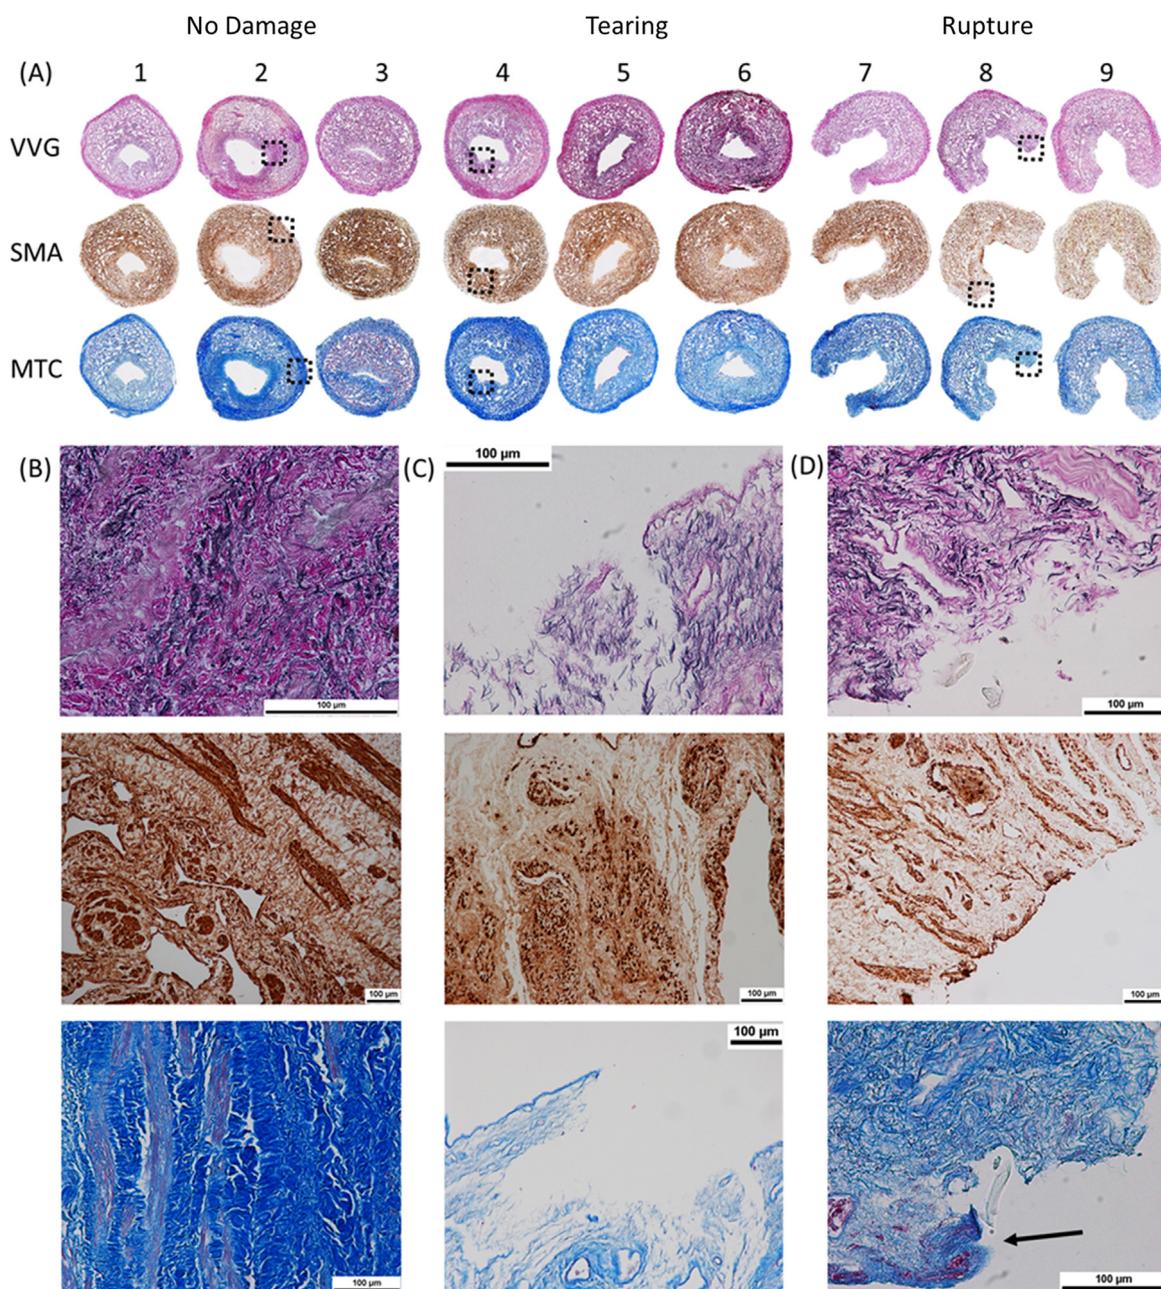


Fig. 3. A) Histological stains depicting the effects of catheter balloon induced trauma on urethral ECM. B) Urethral ECM of samples that sustained no damage despite balloon inflation in the bulbar urethra. Fibres of elastin are dispersed throughout the ECM and are most dense in the middle and inner layers. Long striated muscle fibres are present in the outer layer of the urethra with smooth muscle occurring in the middle layer. Collagen occurs as wavy coiled bundles of fibres in the outer layer of the urethra. C) Splitting of urethral tissue is observed in urethral samples that experienced tearing. Elastin, muscle and collagen fibres are frayed and separated. D) Complete transection of collagen, elastin and muscle fibres is observed in the samples that experienced rupture. Disruption of the epithelial layer is also evident in the MTC stain (indicated with an arrow).

applied to an increased cross sectional area, which will increase with increasing wall thickness. Similarly, samples with a higher collagen content were less likely to experience injury relative to samples with a lower collagen content.

These histological findings also conform to the severity of urethral injury that results from traumatic UC. In ruptured urethras, collagen, elastin and muscle fibres were completely transected thus indicating the long-term potential for urethral stricture disease. Urethral stricture occurs due to scarring of the spongy tissue of the corpus spongiosum and most urethral strictures are the result of trauma. When urethral epithelium is breached, the scarring process extends through the tissues of the corpus spongiosum into adjacent tissues leading to contraction of

the scar and reduced urethral lumen. These mechanical and histological findings demonstrate that traumatic UC transects urethral epithelium which is a major risk factor for scar and subsequent stricture formation.

These findings are clinically relevant as millions of urinary catheters are inserted annually and iatrogenic urethral injuries are a potentially preventable source of injury in patients (Manalo et al., 2011) (Wagner et al. 2016, Azar et al. 2016, Wu et al. 2012). Iatrogenic complications from UC are associated with medicolegal implications, financial penalties, longer inpatient stays and long-term urethral stricture disease. In addition to short-term and long-term iatrogenic morbidity and monetary loss, urethral injuries lead to an increased burden on urological resources, inpatient beds and skill use (Wagner et al. 2016,

Azar et al. 2016, Wu et al. 2012). Recently, the incidence, cost, complications and clinical outcomes of iatrogenic urethral catheterisation injuries was prospectively monitored across 2 tertiary referral teaching hospitals and the incidence of urethral trauma was 6.7 patients per 1000 patients catheterised. Furthermore, 81% of patients with urethral trauma sustained a Clavien-Dindo complication \geq grade 2 and the cost of managing these inpatient complications was €335,377 over a 6-month period (Davis et al., 2017a). To decrease or eliminate the risk of urethral injury during UC, urologists must be willing to advocate for safer urethral catheter design modifications using mechanical and histological findings derived from appropriate models such as those outlined in this study. Adjustments and improvements to catheter mechanics will likely result in an incremental decrease in iatrogenic urethral trauma.

A potential limitation of this study is that urethral samples in the present study were embedded solely in the corpus spongiosum without the supportive corpus cavernosum, fascial dartos and skin layers. These supporting structures reinforce the urethra and the inflation pressures leading to urethral injury identified in this study may underestimate *in vivo* inflation injury pressures. However, intentional inflation of a catheter balloon in an *in vivo* urethra is unethical. Therefore, the novel transgender model described herein provides a reasonable estimation of inflation pressure thresholds with an additional safety factor incorporated as the supporting structures that reinforce the urethra *in situ* are absent. Furthermore, this study only considers the bulbar urethra. Future studies should seek to inflate catheter anchoring balloons in the membranous and prostatic urethra, two other common locations for misplaced catheter inflation. However, these urethral regions are retained by the patient during transgender surgery and therefore a separate model to the one described in this study is required. Although samples were obtained from patients engaged in long term oestrogen hormone treatment, there is no literature to suggest that hormone therapy alters the structure and mechanics of the urethra or surrounding tissues. Additionally, oestrogen has been identified in the penises of men not engaged in hormone therapy and is believed to play a role in blood vessel regulation (Dietrich et al., 2004). Therefore, the effects of hormone treatment on sample mechanics and composition in this study were not considered. It is also important to acknowledge that the sample size examined in this study is relatively limited and that there is considerable variance in patient age. However, patient age was not found to correlate significantly with any of the mechanical, compositional or geometrical sample parameters determined in this study.

5. Conclusion

In human male urethras, this study demonstrate that urethral injury occurs at an external urethral diametric stretch \geq 1.26 or with balloon inflation pressures \geq 120kPa. These findings are important as contemporary catheters routinely generate inflation pressures that are significantly greater. This means that iatrogenic urethral injuries will continue to occur unless safety mechanics are introduced to standard

urinary catheters using mechanical and histological findings derived from appropriate models such as those outlined in this study.

Acknowledgements

This work was funded in part by the European Union's Horizon 2020 research and innovation programme under the Marie Skłodowska-Curie grant agreement No 708867 awarded to EC.

Appendix A. Supplementary material

Supplementary data associated with this article can be found in the online version at <http://dx.doi.org/10.1016/j.jmbbm.2018.04.015>.

References

- Azar, R., Shadpour, P., 2016. In vivo trial of a novel Atraumatic urinary Catheter design for prevention of Catheter-induced trauma. *J. Endourol.* 30 (7), 822–827.
- Davis, N.F., Mooney, R.O.C., Cunnane, C.V., Cunnane, E.M., Thornhill, J.A., Walsh, M.T., 2015. Preventing urethral trauma by inadvertent inflation of catheter balloon within the urethra during catheterisation: Evaluation of a novel safety syringe after correlating trauma with urethral distension and catheter balloon pressure. *J. Urol* ([Internet]. Elsevier Ltd), Available from: <<http://linkinghub.elsevier.com/retrieve/pii/S0022534715003936>>.
- Davis, N.F., Quinlan, M.R., Bhatt, N.R., Browne, C., Macraith, E., Manecksha, R., et al., 2017a. Trauma/reconstruction/Diversion Incidence, cost, complications and clinical outcomes of Iatrogenic urethral catheterization injuries: a prospective multi-Institutional study overview of study design. *J. Urol.* 196 (5), 1473–1477.
- Davis, N.F., Cunnane, E.M., Mooney, R.C., Manecksha, R.P., Thornhill, J.A., Walsh, M.T., 2017b. Quantification of user and manufacturer variability and mitigation of variability by flow resistance. *Urology* 1–6. ([Internet]. Elsevier Inc). Available from: <http://dx.doi.org/10.1016/j.urol.2016.11.037>.
- Dietrich, W., Haitel, A., Huber, J.C., Reiter, W.J., 2004. Expression of estrogen receptors in human corpus cavernosum and male urethra. *J. Histochem. Cytochem.* 52, 355–360.
- Ebenstein, D.M., Coughlin, D., Chapman, J., Li, C., Pruitt, L.A., 2009. Nanomechanical properties of calcification, fibrous tissue, and hematoma from atherosclerotic plaques. *J. Biomed. Mater. Res - Part A* 91 (4), 1028–1037.
- Kashefi, C., Messer, K., Barden, R., Sexton, C., Parsons, J.K., 2008. Incidence and prevention of iatrogenic urethral injuries. *J. Urol.* 179, 2254–2258.
- Manalo, M., Lapitan, M.C.M., Buckley, B.S., 2011. Medical interns' knowledge and training regarding urethral catheter insertion and insertion-related urethral injury in male patients. *BMC Med. Educ.* 73.
- O'Leary, S.A., Healey, D.A., Kavanagh, E.G., Walsh, M.T., McGloughlin, T.M., Doyle, B.J., 2014. The biaxial biomechanical behavior of abdominal aortic aneurysm tissue. *Ann. Biomed. Eng.* 42 (12), 2440–2450.
- Simhan, J., 2015. Reducing iatrogenic urethral trauma. *J. Urol.* 194 (4), 871–872.
- Sullivan, J.F., Forde, J.C., Thomas, A.Z., Creagh, T.A., 2014. Avoidable iatrogenic complications of male urethral catheterisation and inadequate intern training: a 4-year follow-up post implementation of an intern training programme. *Surgeon* 2–5.
- Thomas, A.Z., Giri, S.K., Meagher, D., Creagh, T., 2009. Avoidable iatrogenic complications of urethral catheterization and inadequate intern training in a tertiary-care teaching hospital. *BJU Int.* 104, 1109–1112.
- Villanueva, C., Hemstreet, G.P., 2008. Difficult male urethral catheterization: a review of different approaches. *Int. Braz. J. Urol.* 401–412.
- Wagner, K.R., Bird, E.T., Coffield, K.S., 2016. urinary catheterization: a paradigm shift in difficult urinary catheterization. *Curr. Urol. Rep.*
- Wu, A.K., Blaschko, S.D., Garcia, M., McAninch, J.W., Aaronson, D.S., 2012. Safer urethral catheters: how study of catheter balloon pressure and force can guide design. *BJU Int.* 109, 1110–1114.